

Transferring your Omnipod DASH® Settings




In order to set up your replacement Omnipod DASH® Personal Diabetes Manager (PDM) you need your current insulin settings. To retrieve your insulin settings from your current Omnipod DASH® PDM, please follow steps 1–5 below.

When you are ready to set up your replacement Omnipod DASH® PDM please gather the following items:


- Omnipod DASH® PDM currently in-use
- Replacement Omnipod DASH® PDM
- A new Pod
- Insulin
- Alcohol swabs
- A copy of your insulin settings.
You can obtain your insulin settings by either:
 - Checking your current Omnipod DASH® PDM
 - Printing your pump settings report from your Glooko®/Diasend® account
 - Contacting your healthcare provider

It is very important that you accurately enter your insulin pump settings. Entering the wrong settings could lead to serious harm.

Step 1 Write Down Your Blood Glucose Range

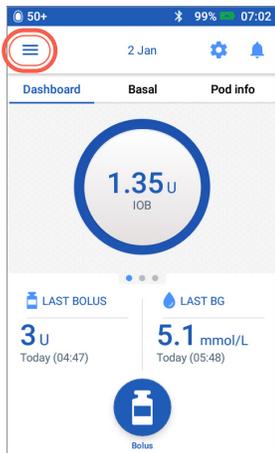

1. From the Home screen tap Menu icon

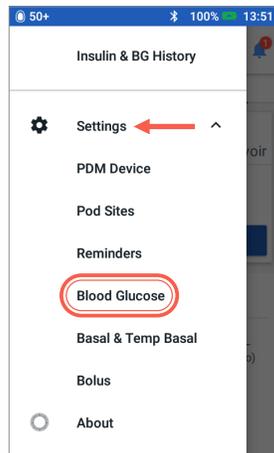


2. Under “Settings” tap Blood Glucose. Write down your BG Goal Range.


BG RANGE		
BG Goal Range:	Lower: _____ mmol/L	Upper: _____ mmol/L




Step 2 Write Down Your Basal Program Settings

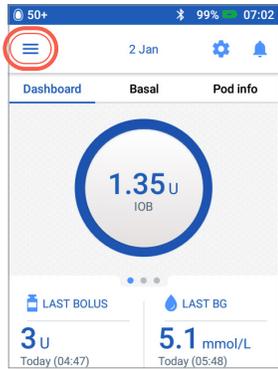

1. From the Home screen tap Menu icon

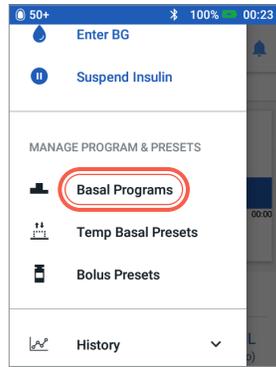

2. Tap "Basal Programs"

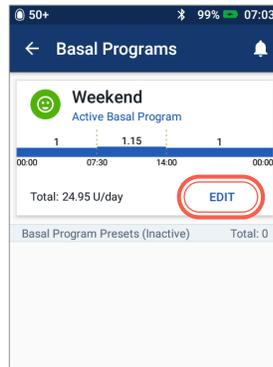

3. Tap "EDIT" to view the basal program. If you have an active Pod, you will need to tap "SUSPEND INSULIN" to view the active basal program. Review Program Name/Tag. Tap "NEXT"




4. Review and write down Basal segments, rates and total basal amount found on this screen. Scroll down to include all segments for the entire 24 hour day. Tap "CANCEL". If you suspended insulin, you must tap "RESUME INSULIN" to restart your basal delivery.

BASAL SETTINGS		
Basal 1 Program (≡ >Settings>Basal Programs) Total Basal _____ U/day	Time Segment	Basal Rate
	12:00am - _____	_____ U/hr
	_____ - _____	_____ U/hr
	_____ - _____	_____ U/hr
	_____ - _____	_____ U/hr
Max Basal Rate (≡ >Settings>Basal & Temp Basal)	_____ U/hr	
Temporary Basal Rate (≡ >Settings>Basal & Temp Basal)	<input type="checkbox"/> ON <input type="checkbox"/> OFF	


Note: If you have additional Basal Programs, you can repeat the steps above for each program.

For your safety, when setting up your replacement DASH® PDM with Basal Programs double-check that the Total Basal amounts MATCH in both PDMs

Step 3 Write Down Your Bolus Settings

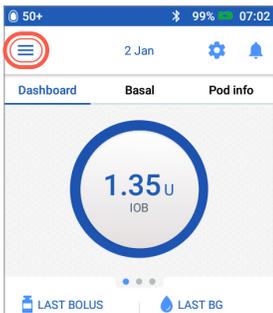


1. From the Home screen tap Menu icon

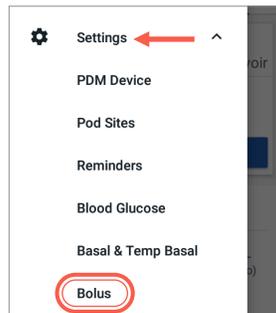

2. Tap "Settings" to expand list. Tap "Bolus"


3. Tap on each Bolus setting. Write down all of the details for each of the settings listed on the table provided here. Remember to scroll down to include all of the Bolus settings.

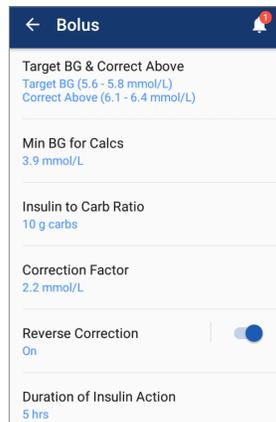


BOLUS SETTINGS (≡ >Settings>Bolus)			
Bolus Calculator	<input type="checkbox"/> ON <input type="checkbox"/> OFF		
Target BG & Correct Above	Time Segment	Target BG	Correct Above
	12:00am - _____	_____ mmol/L	_____ mmol/L
	_____ - _____	_____ mmol/L	_____ mmol/L
	_____ - _____	_____ mmol/L	_____ mmol/L
	_____ - _____	_____ mmol/L	_____ mmol/L
Min BG for Calcs	_____ mmol/L		
Insulin to Carb (IC) Ratio	Time Segment	1 unit of insulin covers	
	12:00am - _____	_____ g	
	_____ - _____	_____ g	
	_____ - _____	_____ g	
	_____ - _____	_____ g	
Correction Factor (CF)	Time Segment	1 unit of insulin decreases BG by	
	12:00am - _____	_____ mmol/L	
	_____ - _____	_____ mmol/L	
	_____ - _____	_____ mmol/L	
	_____ - _____	_____ mmol/L	
Reverse Correction	<input type="checkbox"/> ON <input type="checkbox"/> OFF		
Duration of Insulin Action	_____ hours		
Max Bolus	_____ units		
Extended Bolus	<input type="checkbox"/> ON <input type="checkbox"/> OFF		

Step 4 Reminders


It will be helpful for your routine to use the same Reminders in your replacement Omnipod DASH® PDM

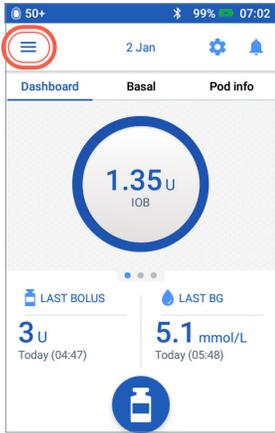

1. From the Home screen tap Menu icon

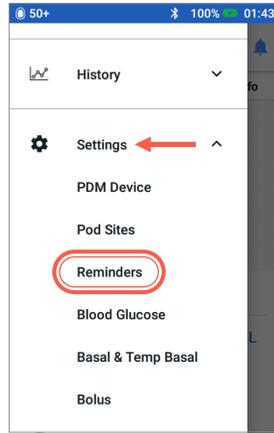

2. Tap “Settings”. Then Tap “Reminders”

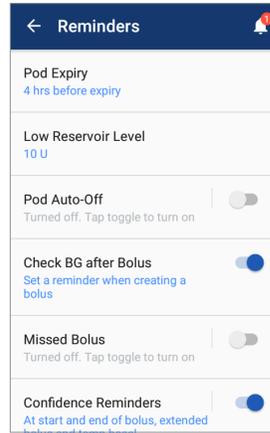

3. Tap on each reminder. Write down all the details of each reminder. Make sure to scroll down to include all the reminders listed

ADDITIONAL SETTINGS – Reminders

Reminders (☰>Settings>Reminders)

Now that you have your insulin pump settings written in this guide, you are ready to follow the First Time Setup steps in your replacement Omnipod DASH® PDM. Remember, it is important that you accurately enter your insulin pump settings. Entering the wrong settings could lead to serious harm. You may also consider asking a friend or family member to double check that you have entered your settings accurately.

After you complete First Time Setup your replacement PDM will ask you to activate a new Pod. If you have not already done so remember to deactivate your Pod from your currently in-use PDM.

Please contact Product Support at 1800 954 074 for any questions about your Omnipod DASH® System.



ALWAYS FOLLOW THE DIRECTIONS FOR USE

Personal Diabetes Manager (PDM) screens are for educational purposes only and should not be considered suggestions for settings.

© 2022 Insulet Corporation. Omnipod, the Omnipod logo, DASH, the DASH logo and Podder are trademarks or registered trademarks of Insulet Corporation in the United States of America and other various jurisdictions. All rights reserved. Glooko® is a trademark of Glooko Inc. and used with permission. The Bluetooth® word mark and logos are registered trademarks owned by the Bluetooth SIG, Inc. and any use of such marks by Insulet Corporation is under license. All other trademarks are the property of their respective owners. The use of third party trademarks does not constitute an endorsement or imply a relationship or other affiliation. INS-ODS-10-2022-00104 V1.0

