


14-Day Summary
06/03/2025-20/03/2025 | Report Generated: 20/03/2025


Time in Ranges

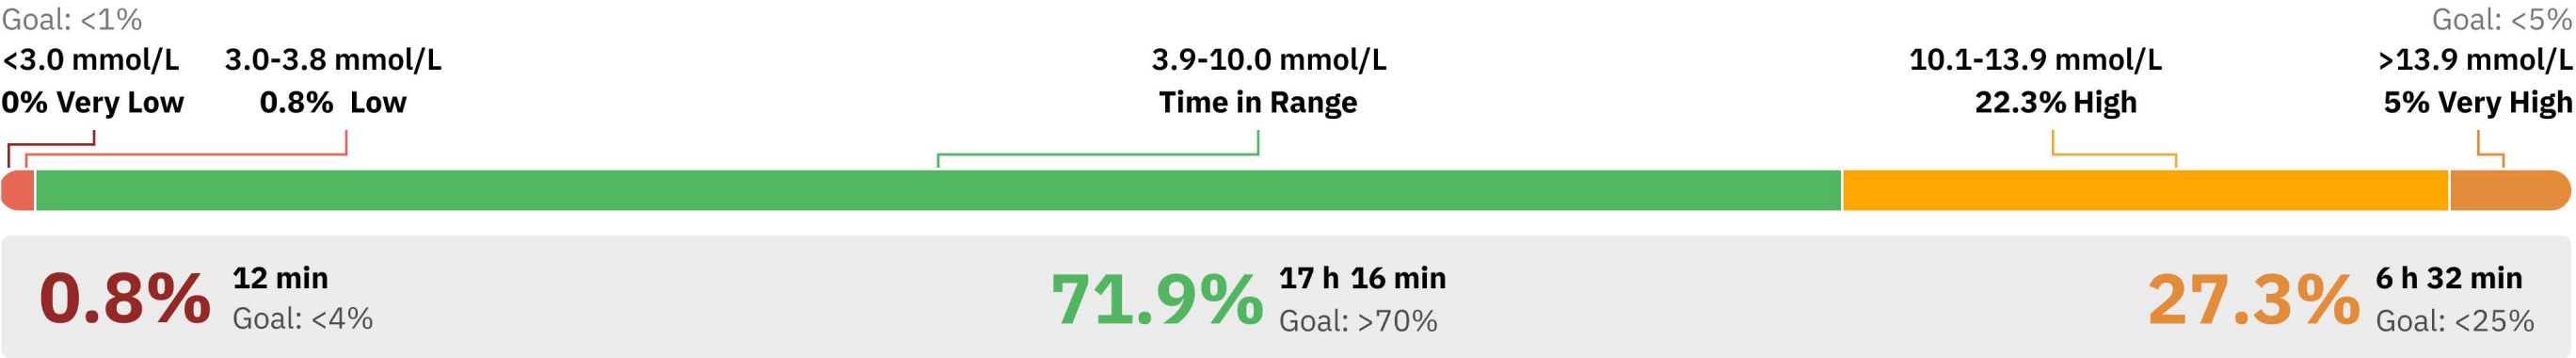

Glucose Metrics		Device Use Omnipod 5 & Dexcom G7	
Average Glucose	8.7 mmol/L	96% 4% Automated Mode Activity 3% Limited 1% Manual Mode	Active Pod Wear Time 99%
Glucose Variability (CV*)	30.4% Goal: ≤36% *Coefficient of variation		Avg Pod Wear Time 2.4 Days (58 hrs)
Glucose Mgmt Indicator (GMI)	7.1% Goal: <7%		Connected Sensor Time 99%
Standard Deviation (SD)	2.6 mmol/L		

Ambulatory Glucose Profile (AGP)

AGP is a summary of glucose values from the report period, with median (50%) and other percentiles shown as if they occurred in a single day.

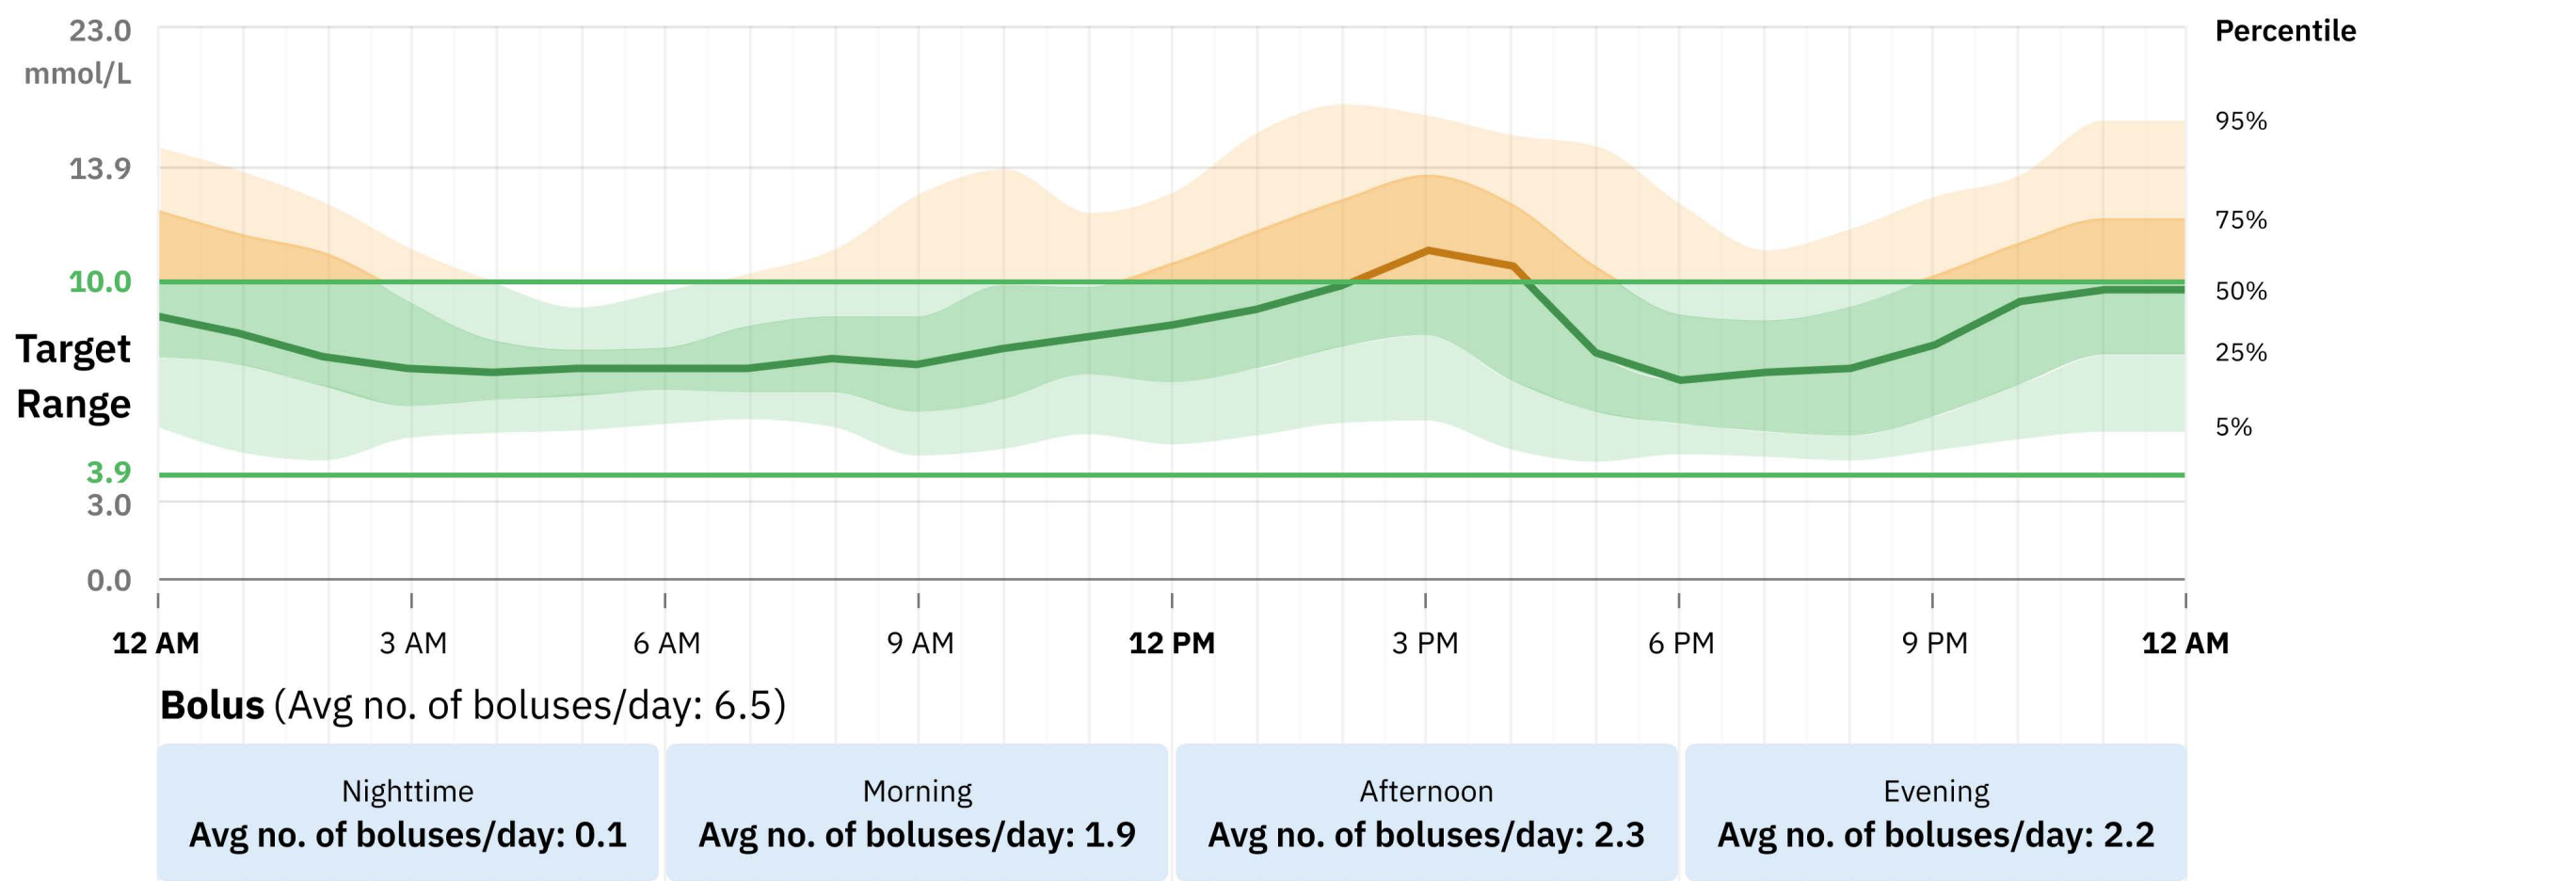


Omnipod 5 Settings

Duration of Insulin Action 3 hrs		Target Glucose (mmol/L)
6.1		Correct Above (mmol/L)
6.1		Insulin to Carb Ratio (unit:grams)
1:9		Correction Factor (unit:mmol/L)
1:2.8		
1:10		
1:8		
12 AM	3 AM	6 AM
9 AM	12 PM	3 PM
6 PM	9 PM	12 AM

Insulin Summary


Avg Total Daily Insulin: 27.1 U

Basal/Day
54%
14.5 U

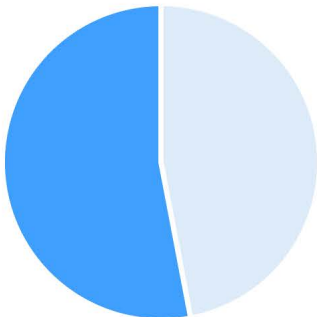

Bolus/Day
46%
12.6 U

Bolus Type

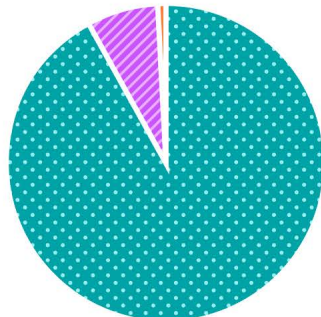

Meal (may include correction)	92.1%	11.6 U
Correction Only	7.1%	0.9 U
Manual	0.8%	0.1 U

Diet

Avg carbs/day
107g

Avg no. of carb entries/day
5.4

Avg no. of boluses/day: 6.5

User override: 4% of total boluses (4 boluses over 14 days)

Jane Smith

DOB: 21/11/1988 (36 years old)

14-Day Daily Report

06/03/2025-20/03/2025 | Report Generated: 20/03/2025

Legend

Glucose

- Sensor Value and Trend
- Manually Entered
- Target Glucose

Bolus

- User Override Up
- User Override Down
- Extended


Insulin Delivery

- Meal Bolus
- Correction Bolus Only
- Manual Bolus


Pod

- Automated
- Manual
- Max Delivery
- Insulin Paused
- Temp Basal
- Pod Change


Thursday, 06/03/2025

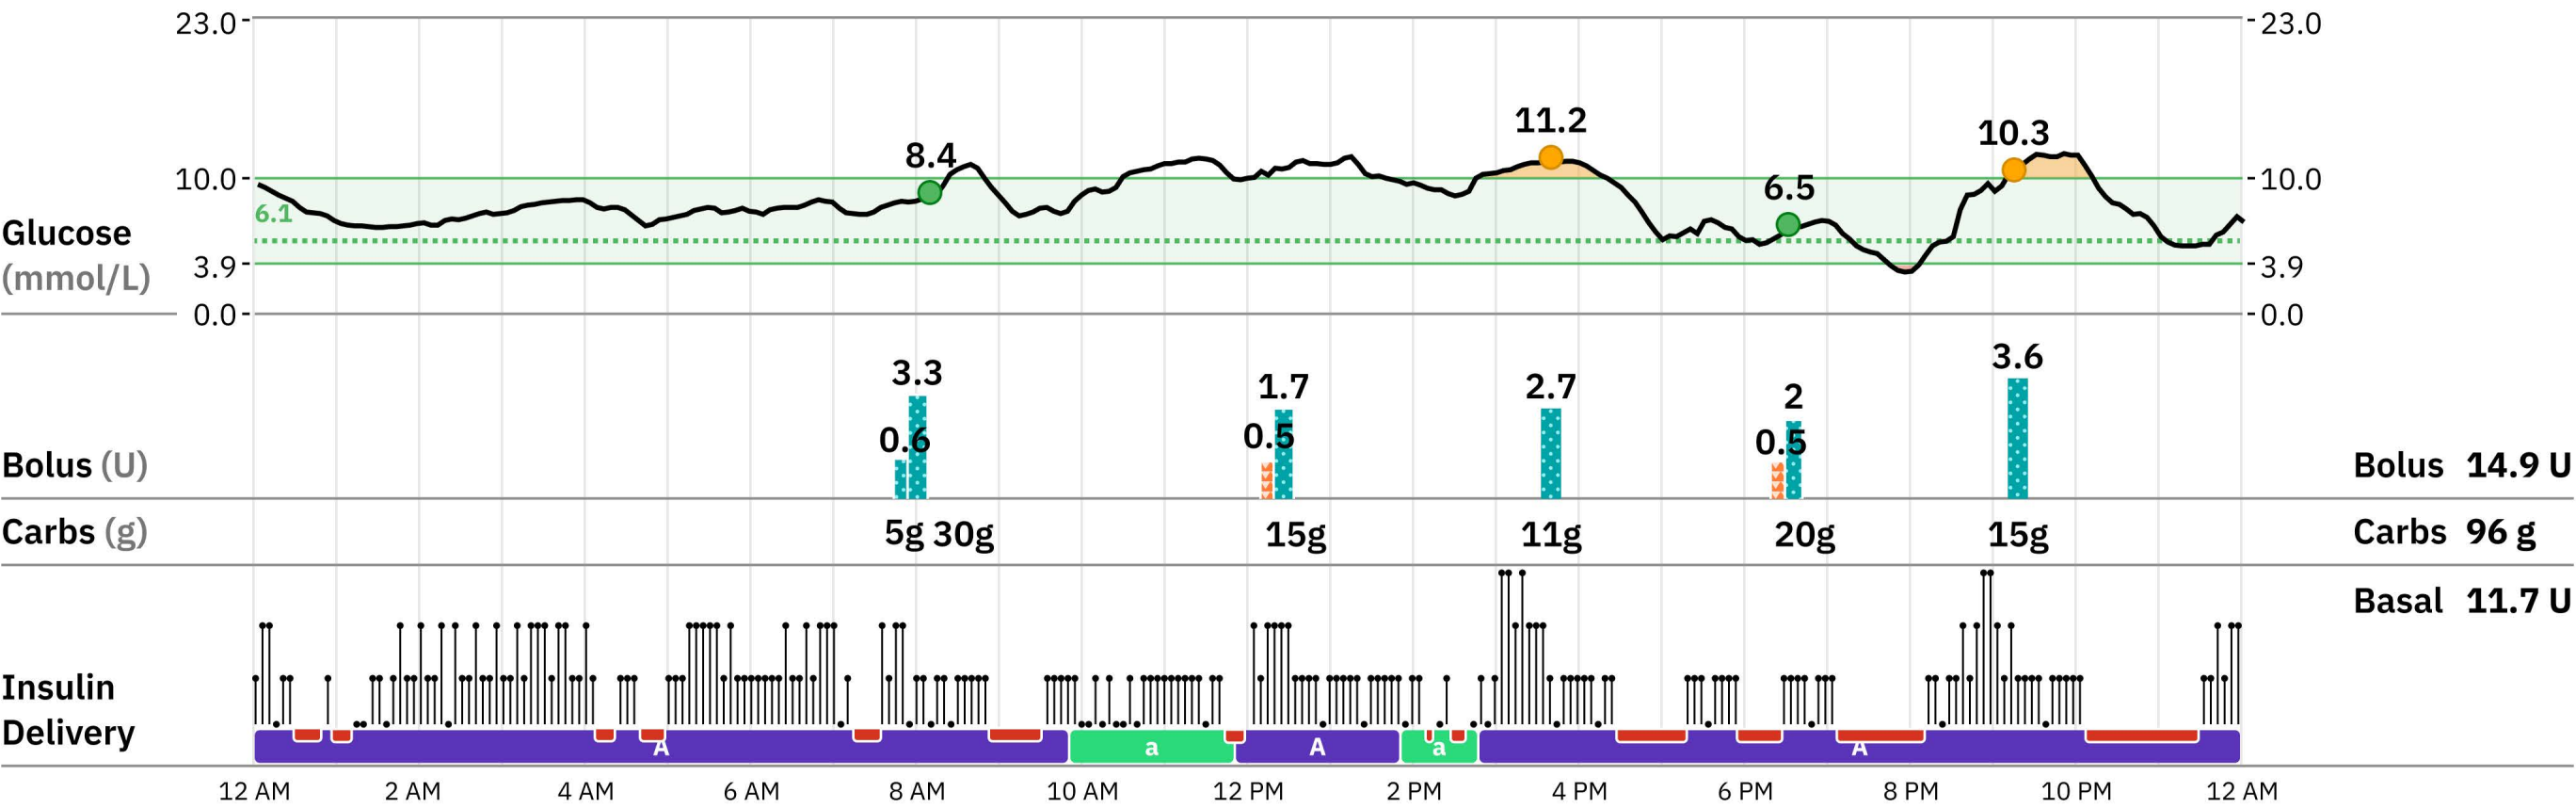

Friday, 07/03/2025

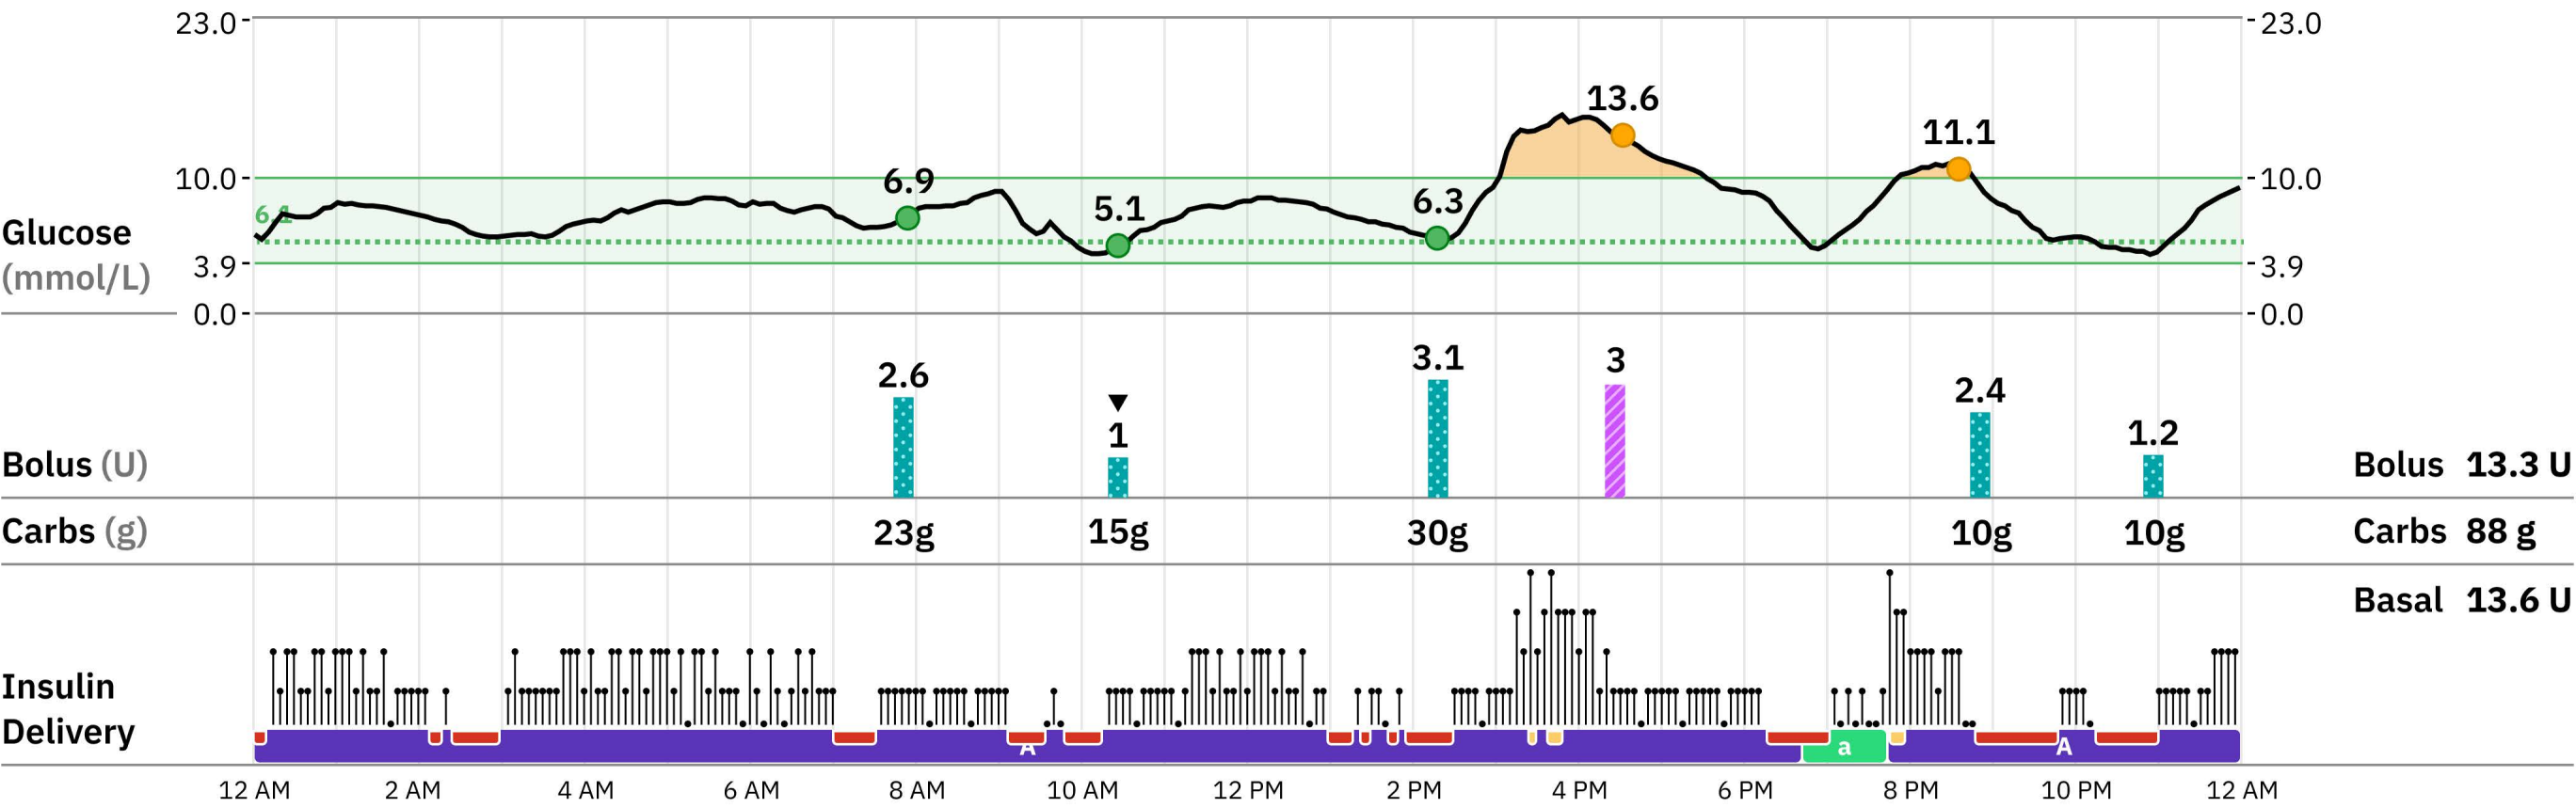

Saturday, 08/03/2025

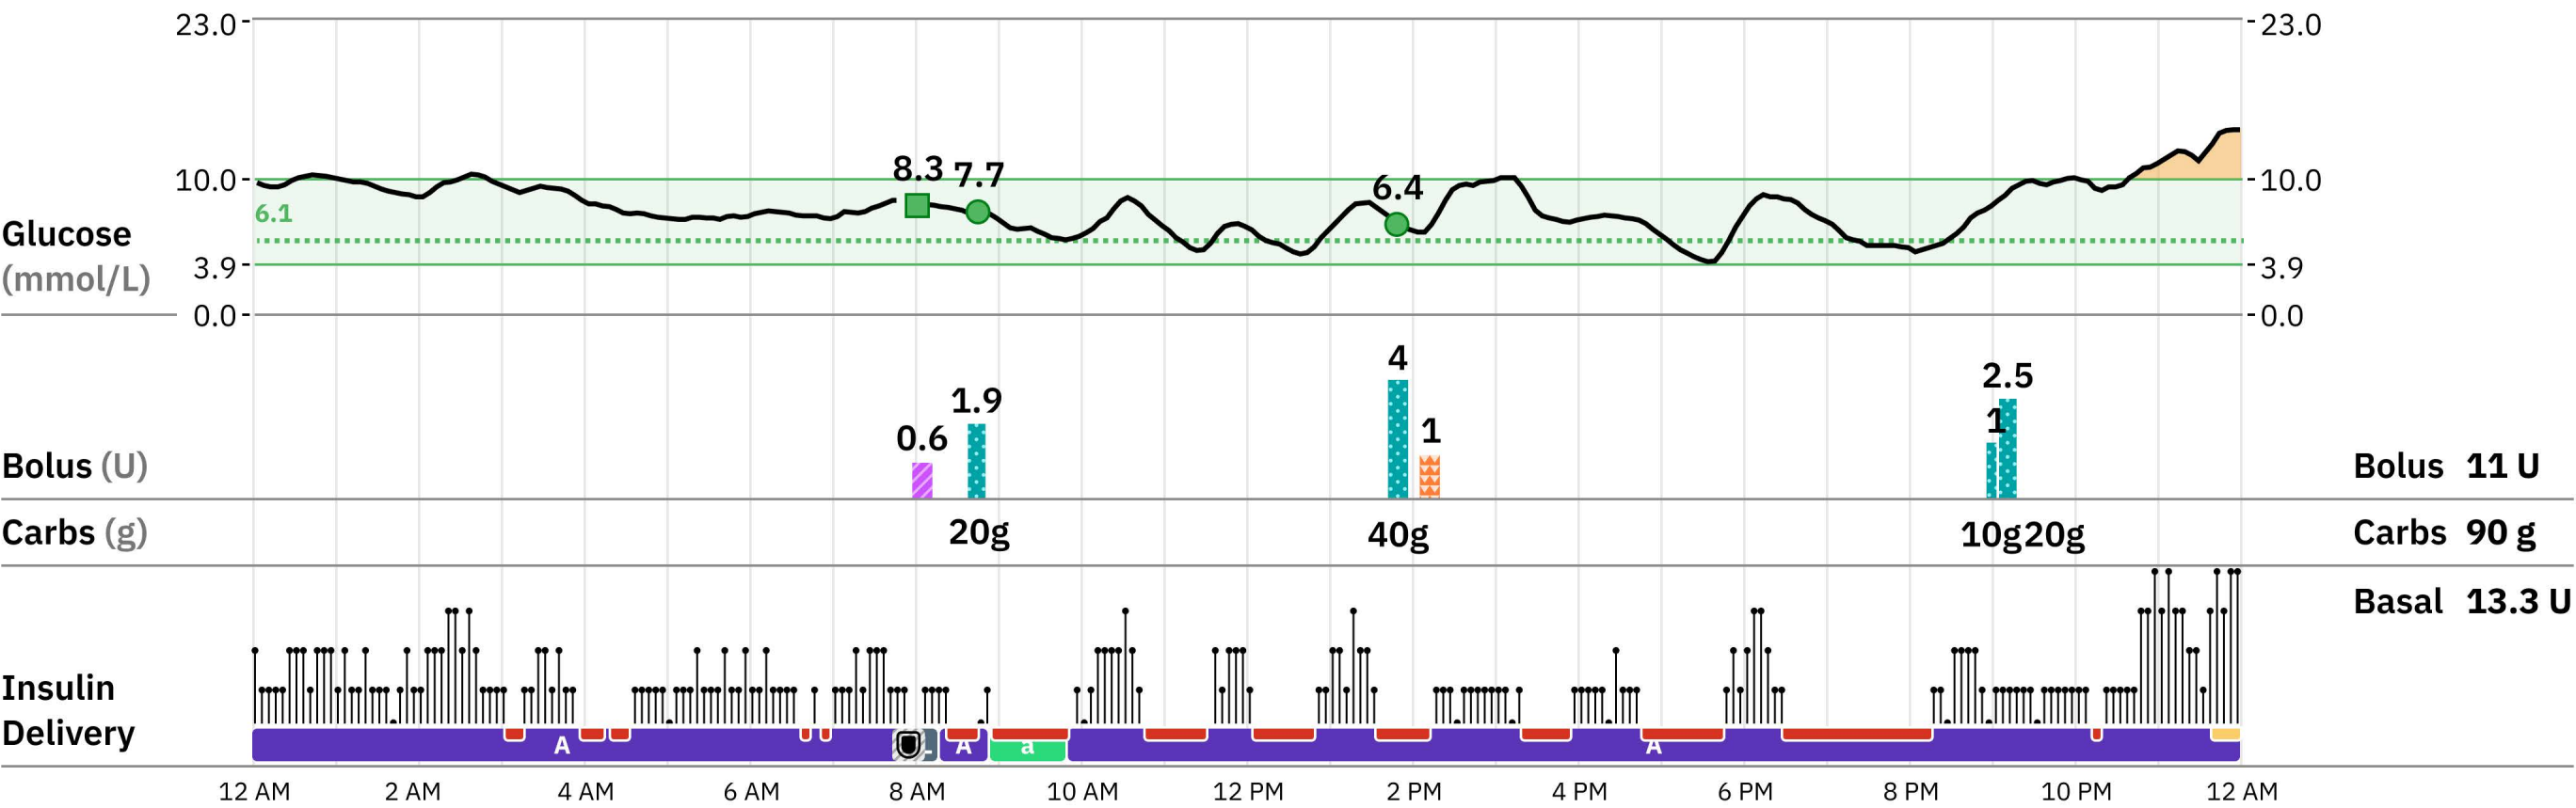

Omnipod 5 Settings

SN: 01040802-000015341 | Report Generated: 20/03/2025 | This page reflects the most recent pump settings

Basal Settings

Changing Basal Programmes only impacts Manual Mode basal delivery.

Max Basal Rate 3 U/hr			
Basal Programmes			
	Start Time	End Time	Basal Rate
Basal 1 (Active)	12:00 AM	7:00 PM	0.6 U/hr
	7:00 PM	12:00 AM	0.85 U/hr
	Total Basal 15.65 U/day		
Temporary Basal Enabled ON			

Bolus Settings

When using Automated Mode, the main adjustable setting that directly impacts automated insulin delivery is Target Glucose. The SmartBolus Calculator settings below impact suggested bolus doses in both Automated and Manual Mode.

	Start Time	End Time	Target Glucose	Correct Above
Target Glucose & Correct Above	12:00 AM	12:00 AM	6.1 mmol/L	6.1 mmol/L
	Start Time	End Time	1 U of Insulin Covers	
Insulin to Carb (IC) Ratio	12:00 AM	4:00 PM	9 g of carbs	
	4:00 PM	9:00 PM	10 g of carbs	
	9:00 PM	12:00 AM	8 g of carbs	
	Start Time	End Time	1 U of Insulin Lowers Glucose By	
Correction Factor	12:00 AM	12:00 AM	2.8 mmol/L	
Duration of Insulin Action	3 hours			
Max Bolus	8 U			
Extended Bolus	ON			
Min Glucose for Calculation	3.9 mmol/L			
Reverse Correction	OFF			